


At-F Anti Aging, IOME Non Invasive, Non Laser Medical Device Clinically Tested, Proven Results

OF USERS

OF USERS WRINKLES SKIN

*Based on results of a clinical study in 34 patients, measuring improvement in Fitzpatrick Wrinkle Scale at 3 months compared to baseline.



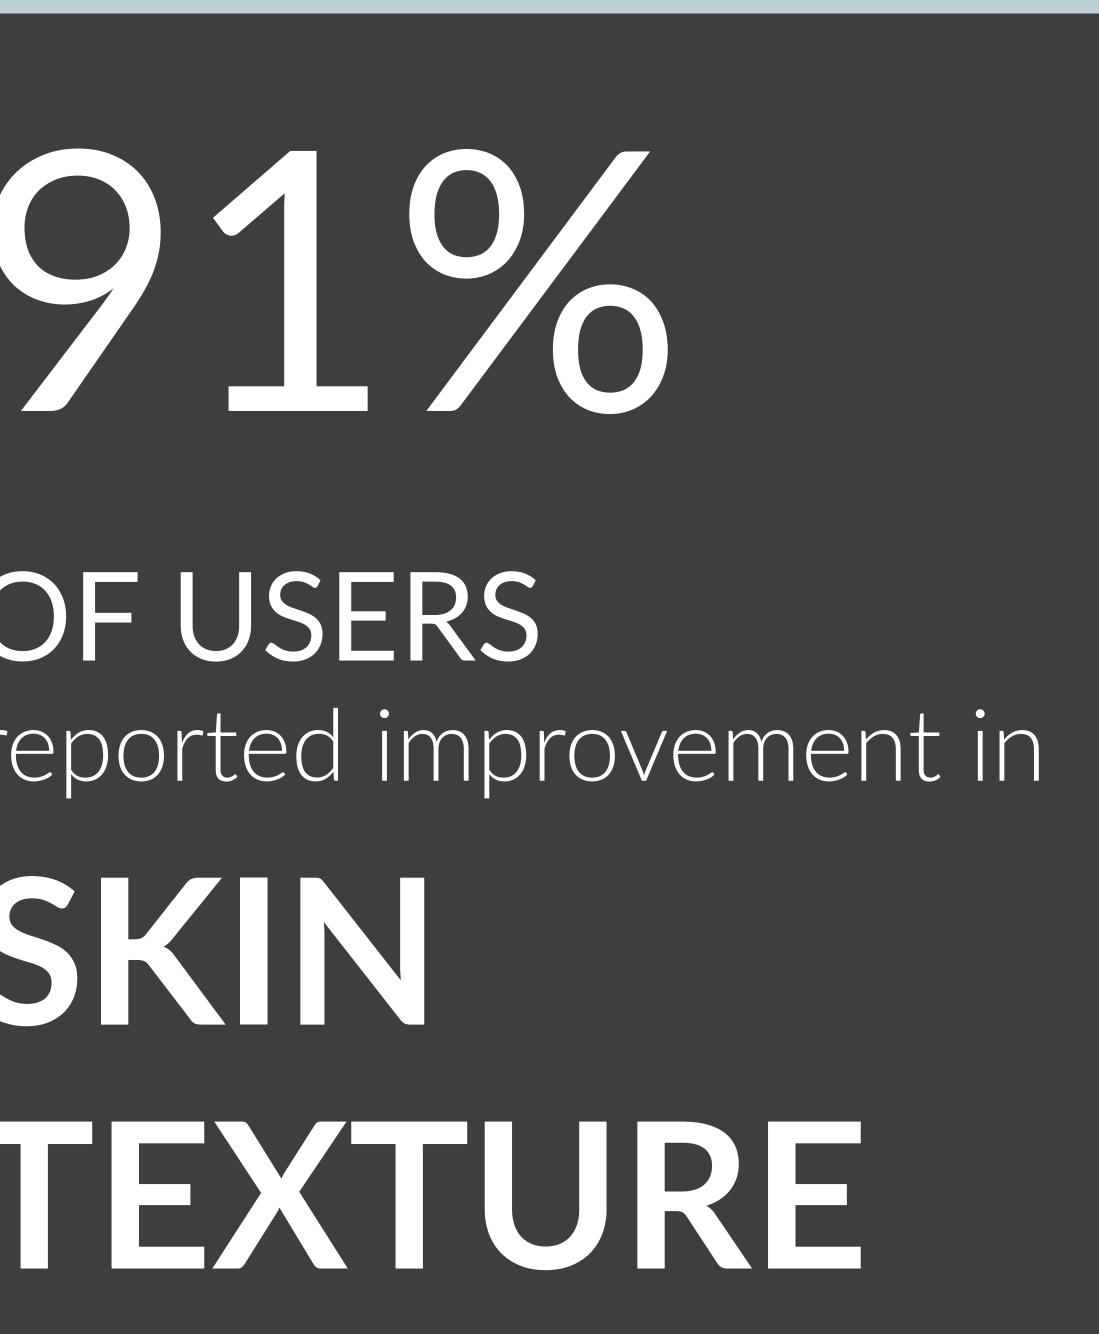



OF USERS reported improvement in **reported improvement in reported improvement in** reported improvement in





OF USERS

PIGNENTS

1







www. avologi.com